




Concrete base at floor level
(210X100 and 180X70 cm)
Concrete base 15 cm thick 1.5 m wide with finished top
Do not include steel bars in the 8 drilling points.

UPS 100 kva is needed
Cables from power panel to be installed thickness needed 35mm 3 phases + neutral + ground
Circuit breaker must be 3 phase + neutral 120 amp
Ground testing should be done less than 1 ohm


NB: Do not include steel bars
in the 8 drilling points.
Leave free area of about 10X10 cm

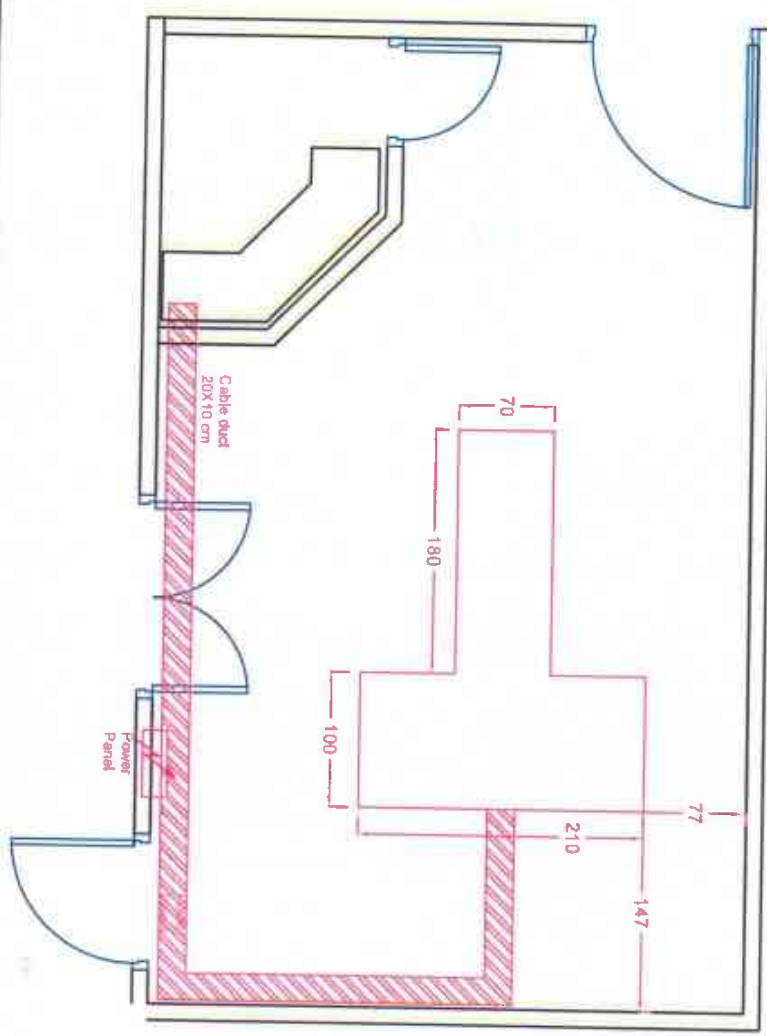

Drawn by : Domis Otayek
Signature :

Rachaya Gov Hosp
Neuviz ACE 64
Concrete

Date: 13 JUL 2026
Scale : 1/50
Dwg # : 2/3

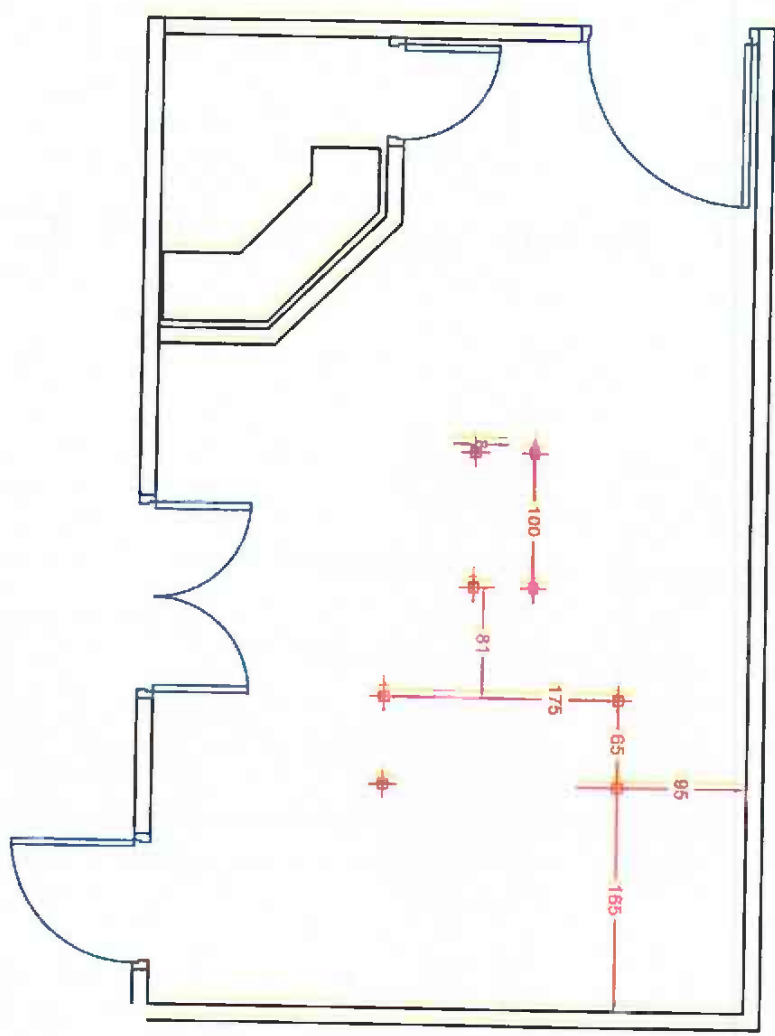

medconsul
middle east s.a.r.l.

Drawn by : **Domis Otayek**
Signature :

Rachaya Gov Hosp


Neuviz ACE 64

Drilling

Date: **13 JUL 2026**

Scale : **1/50**

Dwg # : **3/3**

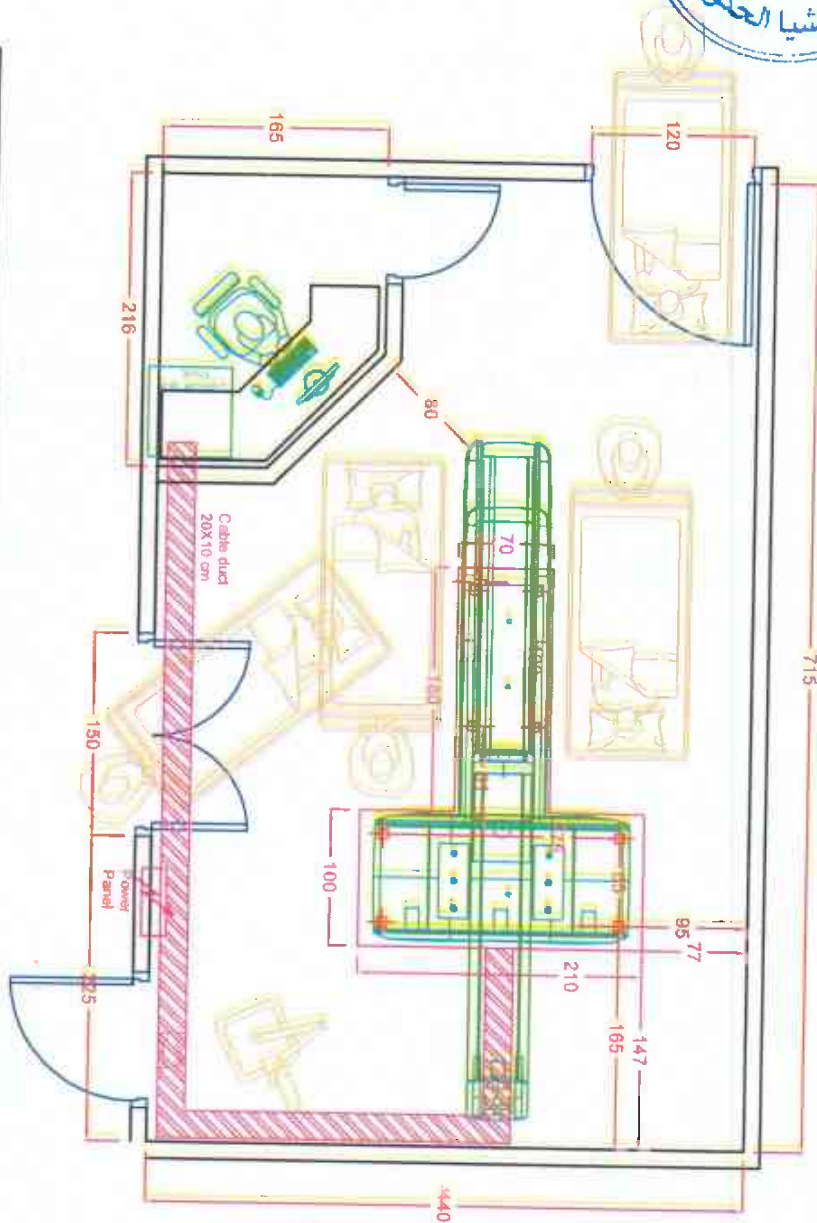

medconsul
middle east s.a.r.l

Drawn by : Domis Otayek

Signature :

Rachaya Gov Hosp

Neuviz ACE 64

All layers

Date: 13 JUL 2026

Scale : 1/50

Dwg # : 3/3